



# Operation Manual for Sensor Interface SI-ETH





# 1 Contents

|           |  |           |
|-----------|--|-----------|
| <b>1</b>  | <b>Contents .....</b>  | <b>2</b>  |
| <b>2</b>  | <b>Imprint.....</b>  | <b>3</b>  |
| <b>3</b>  | <b>Remarks.....</b>  | <b>4</b>  |
| 3.1       | Designation of the Remarks .....   | 4         |
| 3.2       | Safety Notes .....   | 4         |
| 3.2.1     | General References.....  | 4         |
| 3.2.2     | Intended Purpose, Improper Usage .....   | 4         |
| 3.2.3     | Installation Notes .....   | 4         |
| 3.2.4     | Disturbance, Maintenance and Repair Notes.....                                   | 5         |
| <b>4</b>  | <b>Preamble.....</b>   | <b>6</b>  |
| 4.1       | Product Description .....  | 6         |
| 4.2       | Safe and Correct Use .....   | 6         |
| <b>5</b>  | <b>Technical Details of the SI-ETH.....</b>                                      | <b>7</b>  |
| 5.1       | Configuration of the Connections .....   | 7         |
| 5.2       | Adjustment of the Second-Order Low Pass Filter for each Sensor Channel .....     | 7         |
| 5.2.1     | Changing via VS2 .....   | 7         |
| 5.2.2     | Changing via VS .....  | 7         |
| 5.2.3     | Changing via Self-programmed (own) Software.....                                 | 7         |
| <b>6</b>  | <b>Pin Assignments.....</b>  | <b>8</b>  |
| 6.1       | Pin Assignment for Strain Gauge Sensors with mV Signal .....                     | 8         |
| 6.2       | Pin Assignment for Active Sensors with $\pm 5$ V or with $\pm 10$ V Signal ..... | 8         |
| 6.3       | Pin Assignment for Active Current Sensors with 0 .. +20 mA Signal .....          | 8         |
| 6.4       | Pin Connection for the ETH-Interface.....  | 8         |
| <b>7</b>  | <b>Other Application Examples.....</b>   | <b>9</b>  |
| 7.1       | Multi-Component Sensor M-2354 Force and Torque (Strain Gauge/ Strain Gauge)..... | 9         |
| 7.2       | Displacement Sensor Potentiometric (supplied from the SI-ETH) .....              | 9         |
| <b>8</b>  | <b>Debugging .....</b>   | <b>10</b> |
| <b>9</b>  | <b>Specifications .....</b>  | <b>11</b> |
| <b>10</b> | <b>Continuative Documents .....</b>  | <b>12</b> |
| <b>11</b> | <b>Notes .....</b>   | <b>13</b> |



## 2 Imprint

|                      |  |
|----------------------|--|
| Manufacturer, Place  | Lorenz Messtechnik GmbH, D-73553 Alfdorf.  |
| Valid for...         | SI-ETH series  |
| Copyright            | © 2015 Lorenz Messtechnik GmbH, Alfdorf <sup>1</sup> .                                   |
| Reprint-Interdiction | Reprint, even in extracts, only with written authorization from Lorenz Messtechnik GmbH. |
| Modification         | Technical changes reserved.  |

---

<sup>1</sup> All trademarks or brands used in this document refer only to the respective product or the holder of the trademark or brand. Lorenz Messtechnik GmbH does not raise claims to other than its own trademarks or brands.



## 3 Remarks

### 3.1 Designation of the Remarks

If possible remaining dangers emerge during the operation with SI-ETH, this will be indicated by the following symbols in this operation manual:

**Note:**

Important points to consider

### 3.2 Safety Notes

#### 3.2.1 General References

The enclosed operating instruction is intended for technically qualified personnel who have corresponding knowledge in the field of measurement and industrial process & control technology.

The precise information about all safety notes contained in this operation manual and warnings, as well as its perfect technical implementation are precondition for the safe installation, the initiation, the secure operation and the maintenance of Lorenz Messtechnik GmbH technology devices. For this purpose it is absolutely necessary that all measures are carried out by qualified personnel. All persons concerned with the project planning, installation and service of Lorenz Messtechnik GmbH devices, must be familiar to the security concepts in automatic control and should be qualified in this sense.

For clarity reasons, the enclosed operating instruction cannot represent complete details in all conceivable cases of applications for the handling of Lorenz Messtechnik GmbH devices. Further, we cannot consider the entire types of installation, handling and maintenance. If you wish further information or if special problems occur, which were not, or not at length represented in this operating instruction, contact us, please.

**The oblivion of the safety notes will lead to material damages, body injuries and death.**

**Lorenz Messtechnik GmbH devices may only be operated in accordance with the applications described in this operation manual. Built-in devices may only be operated in appropriate installations.**

With the connection and the initiation of the device, the customer accepts the general sale and delivery conditions of Lorenz Messtechnik GmbH. Further, he accepts eventually incomplete operation manuals. The information described is without guarantee. Errors and changes are reserved.

#### 3.2.2 Intended Purpose, Improper Usage

A Lorenz Messtechnik GmbH device is used for displaying, processing and controlling or regulation of processes. It shall not be used as the only tool for the prevention of dangerous states to machines and plants. Machines and plants must be constructed in such a way, that erroneous states cannot lead to a dangerous situation for the staff (e.g. by independent limit switches, mechanical locking devices). It must be guaranteed in particular that device-operating errors, its malfunction or its breakdown do not lead to great property damages or danger for the staff. Consequently, the device then can be used to prevent the machine or the technical installations from error conditions.

It is also important that the use of devices does not endanger precautions for the safety of technical installations.

Emergency-off settings must remain effective in all operation modes.

#### 3.2.3 Installation Notes

Lorenz Messtechnik GmbH devices must be installed and connected by compliance with the relevant DIN- and VDE-norms. They must be installed in such manner that an unintentional use is adequately excluded. The corresponding hardware and software safety precautions are to be observed in such manner that an interruption of the supply and signal cables cannot lead to an undefined or dangerous state. Supply and signal cables must be installed in such way, that disturbing signals (e.g. inductive or capacitive intersperses) will not cause derogations to the function of Lorenz Messtechnik GmbH devices.



### 3.2.4 Disturbance, Maintenance and Repair Notes

The devices do not contain parts which can be maintained on the customer side. Repairs shall be carried out by Lorenz Messtechnik GmbH exclusively.

If assuming that a safe operation of the device is not possible anymore, it must be closed down and protected against unintentional handling immediately. This, in particular, applies:

- If the device shows visible damages
- If the device is no longer operative
- If parts of the device are loose or slack
- If the connection cables show visible damages

Furthermore, we point out that all obligations of Lorenz Messtechnik GmbH exclusively result from the respective sales contract in which the guarantee has been conclusively settled.



## 4 Preamble

### 4.1 Product Description

The SI-ETH is an amplifier which processes analogous signals and converts these signals into digital measured values. These measured data can be retrieved by the PC by means of the ETH-Interface. The current supply occurs via a separate power supply which is included in delivery.

- Required output voltage: 12 .. 30 V
- Required power supply: 600 mA

The SI-ETH is suitable for the connection and simultaneous value acquisition of two sensors. Depending on the SI-ETH model, respectively four different types of sensor signals can be captured (for specifications see data sheet):

- Strain Gauge Signals:  $\pm 3$  mV/V (equates to  $\pm 30000$  Digits)
- Active Signals with Voltage Input:  $\pm 5$  V (equates to  $\pm 25000$  Digits)
- Active Signals with Voltage Input:  $\pm 10$  V (equates to  $\pm 25000$  Digits)
- Active Signals with Current Input: 0/4..20 mA (equates to 0/4000 . +20000 Digits)

The amplifier type and the resolution are stated on the type label, a type change is only possible by the manufacturer. Hence, only the corresponding sensor type can be connected.



Please consider the signal type. The connection of a wrong signal type can lead to damages.

The measured values are issued in digits (16 bit signed integer format) with leading signs (see above in brackets).

If the SI-ETH is adjusted to a specific sensor, the output value will be stated on the test certificate.

If the SI-ETH is not adjusted to a specific sensor, the output values are adjusted as stated above (in brackets). In this case, the output values are adjusted with a high-precise reference.

The evaluation occurs by the VS2 software which contains following functions:.

- Configuration possibilities for the VS2
- Storage of sensor-related scaling and adjustment data
- Display for the presentation of measured data (actual value, tare value, minimal value and maximal value)
- Presentation of the measured data in a diagram
- Storage of measured data in CSV-format (output configurable)
- Storage of the diagram in BMP-format (output size adjustable)
- Print-out of the diagram (output size defined)
- Presentation of the sensor information

The communication protocol is described in document no. 090110, "A flexible command set for digital sensors and interfaces" which states how to activate the SI-ETH through own software.

### 4.2 Safe and Correct Use



Consider the correct sensor adjustment.



Consider the correct VS2 configuration.



Choose a significant file identification/prefix when storing measured data.



Fasten housing, ground, connect power supply, protect from splash water and do not pull the cable.



## 5 Technical Details of the SI-ETH

### 5.1 Configuration of the Connections

There is no maintainable connection inside the SI-ETH housing. The connection of the power supply unit occurs on the side of the housing. The sensors and the digital interface can be connected through sockets as well.

### 5.2 Adjustment of the Second-Order Low Pass Filter for each Sensor Channel

#### 5.2.1 Changing via VS2

If a SI-ETH was connected, the software offers this option in the tab for measurement adjustments.

#### 5.2.2 Changing via VS

In the advanced mode, the software offers tabs for configuration. The filter frequencies can be adjusted in configuration block STATOR\_OPERATION.

#### 5.2.3 Changing via Self-programmed (own) Software

The adjustment for channel A is stored in bytes 13 and 14 of the configuration block "STATOR\_OPERATION". The value for channel B is stored in bytes 15 and 16. Each byte represents a 16-bit value and corresponds to the cutoff-frequency according following chart:

| Range of values<br>(decimal) | Value<br>(hexadecimal) | Adjusted cutoff-<br>frequency |
|------------------------------|------------------------|-------------------------------|
| $0 \leq X \leq 30$           | 0x001E                 | 30 Hz                         |
| $31 \leq X \leq 300$         | 0x012C                 | 300 Hz                        |
| $301 \leq X \leq 1000$       | 0x03E8                 | 1000 Hz                       |
| $1001 \leq X \leq 65536$     | 0x0BB8                 | 3000 Hz                       |

Please consider that currently adjusted cutoff-frequency will be active after rebooting, only. For further information regarding programming with own software we refer to document 090110, Lorenz protocol "A flexible command set for digital sensors and interfaces".



## 6 Pin Assignments

### 6.1 Pin Assignment for Strain Gauge Sensors with mV Signal

| <u>Description</u> | <u>Pin (6 pole socket)</u> | <u>Color</u> | <u>Remark</u>                                |
|--------------------|----------------------------|--------------|--|
| 0 V / GND          | 1                          | green        | ground reference for 5 V and 12 V excitation |
| 5 V                | 2                          | brown        | excitation for 5 V strain gauge sensors      |
| Shield             | 3                          | shielding    | do not connect shield with sensor housing    |
| Signal +           | 4                          | yellow       | positive signal input                        |
| Signal -           | 5                          | white        | negative signal input                        |
| Control            | 6                          | grey         | if available in sensor                       |

### 6.2 Pin Assignment for Active Sensors with ±5 V or with ±10 V Signal

| <u>Description</u> | <u>Pin (12 pole socket)</u> | <u>Color</u> | <u>Remark</u>                                   |
|--------------------|-----------------------------|--------------|---|
| 0 V / GND          | E                           | green        | ground reference for 4 V and 12 V excitation    |
| 12 V               | F                           | brown        | excitation for 12 V active sensors              |
| Signal +           | C                           | yellow       | signal input                                    |
| Signal -           | D                           | white        | relating to signal input (internally 0 V / GND) |
| Control            | K                           | grey         | if available in sensor                          |
| Shield             | M                           | shielding    | do not connect shield with sensor housing       |

### 6.3 Pin Assignment for Active Current Sensors with 0 .. +20 mA Signal

| <u>Description</u> | <u>Pin (12 pole socket)</u> | <u>Color</u> | <u>Remark</u>                                   |
|--------------------|-----------------------------|--------------|---|
| 0 V / GND          | E                           | green        | ground reference for 12 V excitation            |
| 12 V               | F                           | brown        | excitation for 12 V active sensors              |
| Signal +           | C                           | yellow       | signal input                                    |
| Signal -           | D                           | white        | relating to signal input (internally 0 V / GND) |
| Control            | K                           | grey         | if available in sensor                          |
| Shield             | M                           | shielding    | do not connect shield with sensor housing       |

### 6.4 Pin Connection for the ETH-Interface

| <u>Description</u> | <u>Pin (8 pol. socket)</u> | <u>Color</u> | <u>Remark</u>            |
|--------------------|----------------------------|--------------|--------------------------|
| TX+                | 1                          | orange/white | positive Transmit signal |
| TX-                | 2                          | orange       | negative Transmit signal |
| RX+                | 3                          | green/white  | positive Receive signal  |
| -                  | 4                          | blue         |                          |
| -                  | 5                          | blue/white   |                          |
| RX+                | 6                          | green        | negative Receive signal  |
| -                  | 7                          | brown/white  |                          |
| -                  | 8                          | brown        |                          |

The pin connection of the Ethernet-Interface M12-RJ45 corresponds to the DIN EIA/TIA 568A or 568B Standard.





## 7 Other Application Examples

### 7.1 Multi-Component Sensor M-2354 Force and Torque (Strain Gauge/ Strain Gauge)


The multi-component sensor M-2354 is directly connected to the SI-ETH/DMS/DMS with both outputs. The system allows simultaneous recording of force-torque-courses which chronologically refer to each other.



### 7.2 Displacement Sensor Potentiometric (supplied from the SI-ETH)

A SI-ETH with minimum U5-input is suitable. The accuracy of the displacement measurement is depending on the quality of the reference voltage.

With this set-up, arbitrary measuring variables, depending on displacement measurements, can be recorded and referred to each other.

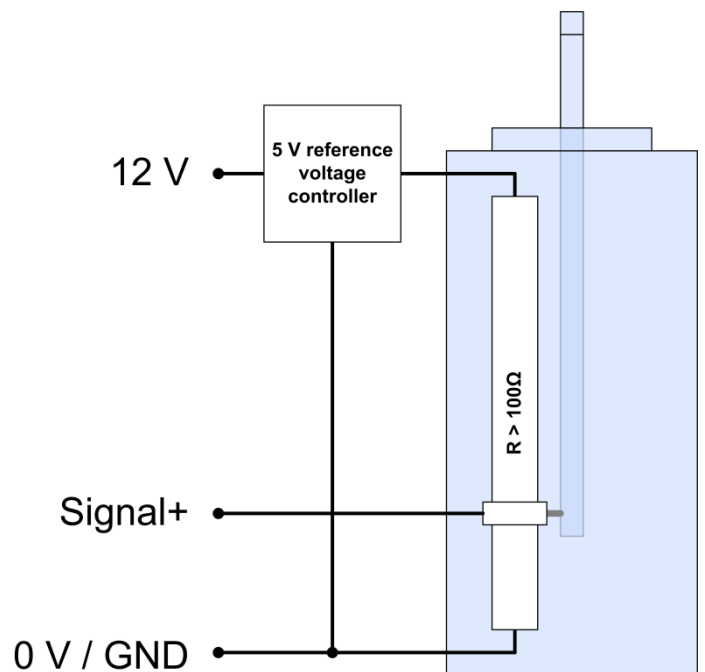

**Output 0..25000 Digits**



## 8 Debugging

This chart helps to find frequent errors and the measures for debugging.

| Error   | Possible Cause  | Debugging   |
|---|---|---|
| A connection to the SI-ETH is not possible.             | Driver incorrectly or not installed.                                    | Install driver package.<br>The first start-up of the SI-ETH must be carried out with administrator rights.  |
|   | Supply voltage is overloaded.   | Check whether the connected sensor corresponds to the specifications of the SI-ETH. If the sensor requires higher current than available for the SI-ETH, this sensor cannot be used together with the SI-ETH. |
|   | Power supply not connected.   | Connect power supply.   |
|   | Supply voltage is shortened.  | Fix the short circuit.  |
| Output signal is at the upper or lower modulation limit | Active-sensor or current-sensor is connected to the strain gauge input. | Check on type label for which input type has been configured for the applied sensor connection.   |
|   | Supply voltage connected to sensor input.                               | Check/correct the pin assignment  |
| Output signal fluctuates (strain gauge)                 | Open sensor input.  | Connect sensor  |
|   | Cut-off frequency adjustment not correctly set.                         | Set cut-off frequency as described in chapter 5.2   |



## 9 Specifications

|                    |                       |                         |                       |                       |                       |
|--------------------|-----------------------|-------------------------|-----------------------|-----------------------|-----------------------|
| <b>Type</b>        | <b>SI-ETH/DMS/DMS</b> | <b>SI-ETH/U5/U5</b>     | <b>SI-ETH/U10/U10</b> | <b>SI-ETH/I20/I20</b> | <b>SI-ETH/DMS/U5</b>  |
| <b>Article-No.</b> | 114907                | 114908                  | 114909                | 114910                | 114911                |
| <b>Input Range</b> | 2* ±3 mV/V            | 2* ±5 V                 | 2* ±10 V              | 2* 0/4...20 mA        | ±3 mV/V; ±5 V         |
| <b>Type</b>        | <b>SI-ETH/DMS/U10</b> | <b>SI-ETH/DMS/I20</b>   | <b>SI-ETH/U5/U10</b>  | <b>SI-ETH/U5/I20</b>  | <b>SI-ETH/U10/I20</b> |
| <b>Article-No.</b> | 114912                | 114913                  | 114914                | 114915                | 114916                |
| <b>Input Range</b> | ±3 mV/V;<br>±10 V     | ±3 mV/V;<br>0/4...20 mA | ±5 V;<br>±10 V        | ±5 V;<br>0/4...20 mA  | ±10 V;<br>0/4...20 mA |

### Evaluation Side

|  |                                   |  |
|--|-----------------------------------|--|
| Supply Power Supply <sup>1</sup><br>Output Power Supply<br>External Supply<br>PoE Supply | Voltage                           | 100...240 V AC<br>24 V DC 1.25 A<br>12...30 V DC < 800 mA<br>or IEEE802.3at Class 4          |
| Sensor Supply  | Strain Gauge<br>U5/U10/I20        | 5 V ≤20 mA<br>12 V ≤200 mA   |
| Measured Values  | Strain Gauge<br>U5/U10<br>I20     | ±3 mV/V = ±30000 Digits<br>±5 V/±10 V = ±25000 Digits<br>0/4...20 mA = 0/4000...20000 Digits |
| Resolution   | Strain Gauge<br>U5<br>U10<br>I20  | 1 mV/V = 10000 Digits<br>1 V = 5000 Digits<br>1 V = 2500 Digits<br>1 mA = 1000 Digits        |
| Zero Point   | Strain Gauge/U5/<br>U10/I20       | 0 Digits   |
| Output Format  |                                   | 16 Bit Signed Int.   |
| Input Resistance   | Strain Gauge/U5/U10<br>I20 burden | >1 MΩ<br>62 Ω  |
| Second-Order Low-Pass Filter   | Hz                                | 30/300/1000/3000   |
| Measuring Rate   |                                   | max. 2500 Meas./s  |
| Temperature Drift  |                                   | 4 Bit/10 K   |
| Linearity Error  |                                   | ±32 Digits   |
| Accuracy   |                                   | ±32 Digits   |

### Miscellaneous

|                              |   |   |
|------------------------------|---|---|
| Cable Length SI-ETH - Sensor |   | 1 m (max. 3 m)  |
| Nominal Temperature Range    |   | 10 ... 40 °C  |
| Service Temperature Range    |   | 0 ... 50 °C   |
| Storage Temperature Range    |   | -10 ... 70 °C   |
| Dimensions (L x B x H)       |   | 125 x 80 x 57 mm  |
| Weight                       |   | 480 g   |
| Level of Protection          |   | IP40  |
| Electrical Connection        | Strain Gauge<br>U5/U10/I20<br>Ethernet <sup>2</sup> | Female socket 6-pin<br>Female socket 12-pin<br>RJS-5EBMMM-SL7E02 (RJ45) |

### Options/ Accessories

| Article-No. | Type                 | Designation  |
|-------------|----------------------|--|
| 110564      | mV/V                 | mV/V adjusted sensitivity  |
| 10302       | KS6                  | Male cable connector 6-pin   |
| 10303       | KS12                 | Male cable connector 12-pin  |
| 10296       | KDM7/A-KS6/A-3m/PVC  | Connection cable for passive sensors, 3 m, with 7-pin female cable connector and 6-pin male cable connector  |
| 10271       | KD6/A-KS6/A-3m/PVC   | Connection cable for passive sensors, 3 m, with 6-pin female cable connector and 6-pin male cable connector  |
| 10279       | KDM8/A-KS12/B-3m/PVC | Connection cable for active sensors, 3 m, with 8-pin female cable connector and 12-pin male cable connector  |
| 10283       | KD12/B-KS12/B-3m/PVC | Connection cable for active sensors, 3 m, with 12-pin female cable connector and 12-pin male cable connector |
| 115523      | PoE12-HP             | PoE power-supply-injector for voltage supply   |

<sup>1</sup> At first delivery power supply in scope of delivery.<sup>2</sup> At first delivery cable SI-ETH evaluation in scope of delivery, cable length 5 m.



## 10 Continuative Documents

Following documents contain reference information about the SI-ETH:

- Document number 090342, "Operation Manual for Sensor Interface SI-ETH (2-Channel)" (German 090341).
- Document number 080758, data sheet "Sensor-Interface with ETH (Type: SI-ETH 2-Channel)" (German 080757).
- Document number 090313, "Operation Manual for Configuration and Evaluation Software LCV-USB-VS2" (German 090312).
- Document number 090344, "Driver Installation Description SI-ETH" (German 090343).
- Document number 090110 Lorenz protocol "A flexible command set for digital sensors and interfaces".



## 11 Notes